


AUG 09 2010

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

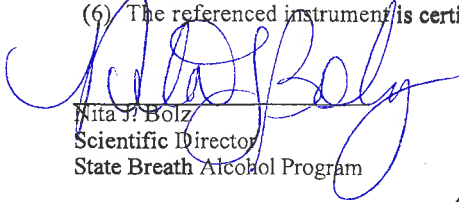
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130187 ✓
Name	Dan Pasquariello	ID#	2620 ✓
		Date	8-03-10 ✓
A	Agency	Dillingham PD	Phone # 842-5354
	Instrument Location	Dillingham PD	
B	Alco S/N	70108 ✓	Target Value .081 ✓
		High Pressure	1200 psi
	Alco Test Values	.083 ✓ 1st Alco	.083 ✓ 2nd Alco
	Signature		
		CB 8/10/10	

(OVER)


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 9<sup>th</sup> day of NOV, 2010.

  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

(Notary Seal Stamp)



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130187

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130187

AUGUST 03, 2010

OPERATOR'S NAME:

PASQUARIELLO, DAN

OPERATOR'S NUMBER: 2620

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: 1234567890

DEPT/AGENCY: DL61

CASE/REPORT: 1234567890

TEST TYPE: V

ALCO TARGET VALUE: .081

ALCO S/N: 70108

### — BREATH ANALYSIS —

.081 ADJUSTED FOR 30.19 in

ALCO TARGET .081 20:56

BLANK TEST .000 20:57

INTERNAL STANDARD VERIFIED 20:57

ALCO TV 30.19 in .083 20:57

BLANK TEST .000 20:58

SUBJECT SAMPLE .000 21:00

BLANK TEST .000 21:01

ALCO TV 30.19 in .083 21:02

BLANK TEST .000 21:02

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130187

AUGUST 03, 2010

TIME 21:06

### — DIAGNOSTIC CHECK —

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 43c

BAROMETER: 30.19 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

### PRINTER TEST

! " # \$ % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~